







AFRICA CENTRE OF EXCELLENCE  
FOR MYCOTOXIN AND FOOD SAFETY  
FEDERAL UNIVERSITY OF TECHNOLOGY, KWARA





AFRICA CENTRE OF EXCELLENCE  
FOR MYCOTOXIN AND FOOD SAFETY  
FEDERAL UNIVERSITY OF TECHNOLOGY, OYO














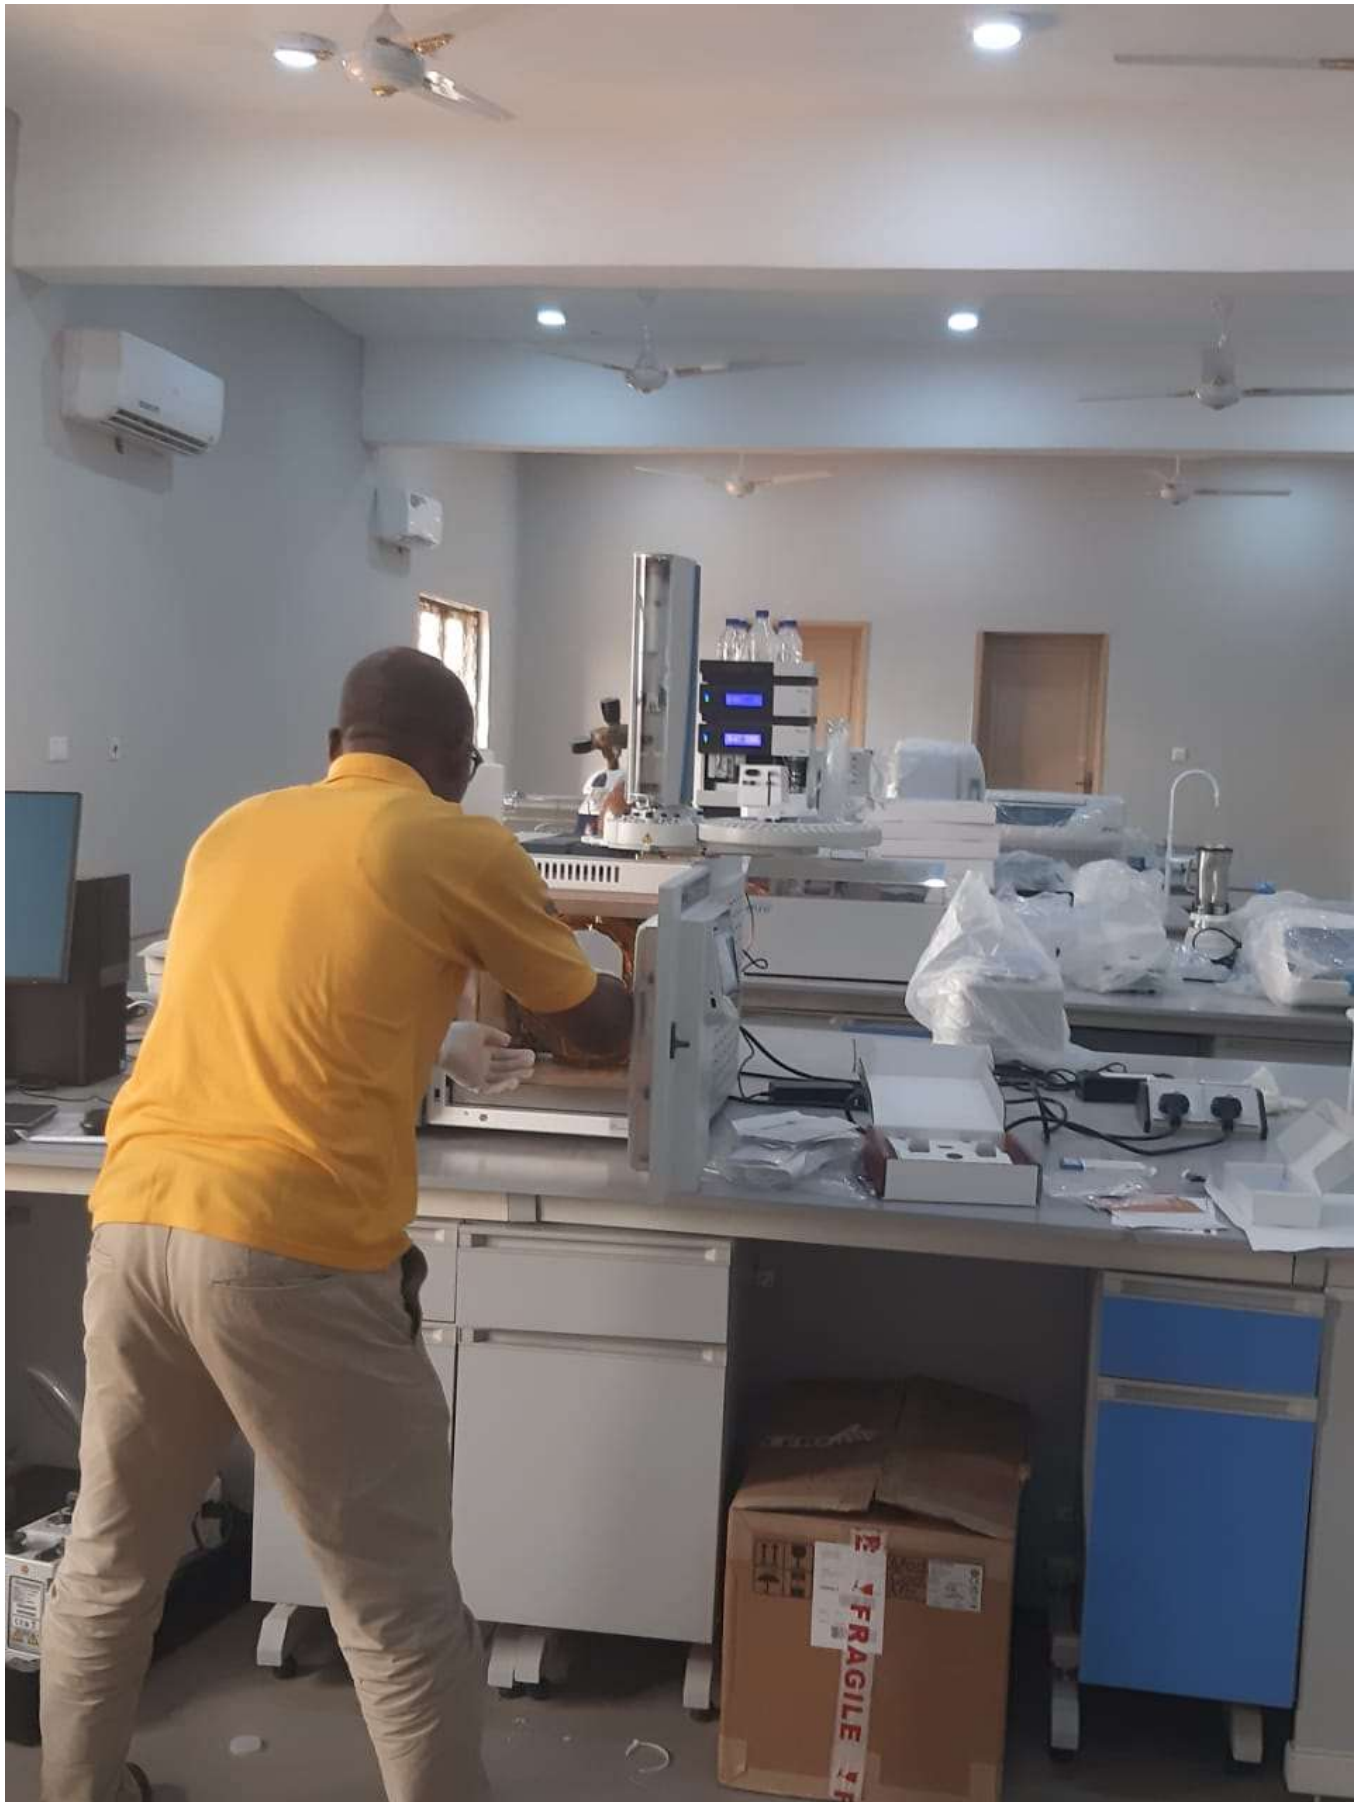























CABINET











FUTMK/ACEMFS/OE/2011/006






FUTUNY/AGEHFS/OE/20/001

FUTUNY/AGEHFS/OE/20/001

FUTUNY/AGEHFS/OE/20/001


DELL  
FUTUNY/AGEHFS/OE/20/001









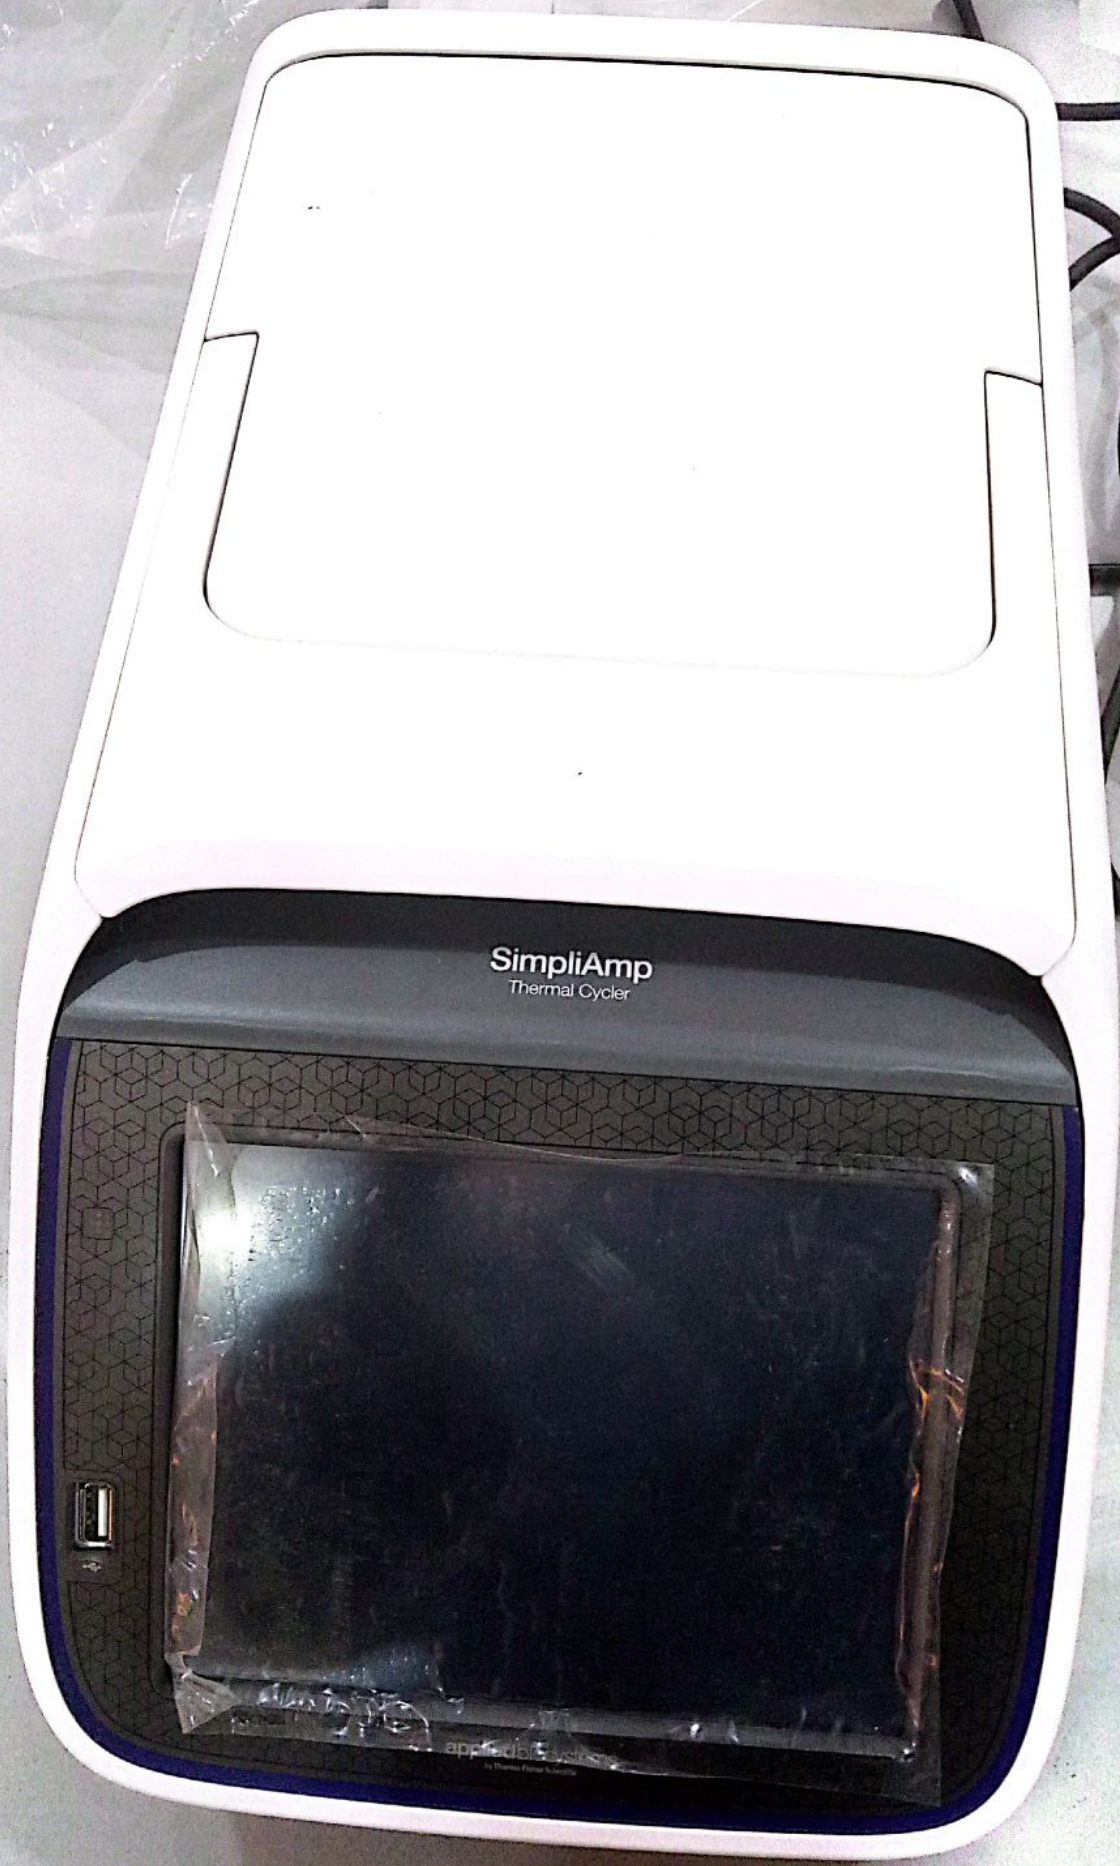

SimpliAmp  
Thermal Cycler

Applied Biosystems  
by Thermo Fisher Scientific



**mrc**

FUTRA/ACEMFS/OE/2011/11/1



POWER









POTMX/ACEMFS/OE/201 100L







FUTMX/ACEMFS/DE/20/1111

thermo**scientific**

ISO 7610  
Single Quadrupole  
Mass Spectrometer

Power Vacuum Heaters Busy

thermo**scientific**

TRACE 1610  
Gas Chromatograph





145 Mar 2010

145 MAR 2010

UVE

145 MAR 2010

145 MAR 2010







Single Stage Vacuum Pump CE

Model:	TW-1K
Free Air Displacement:	2CFM
Ultimate Vacuum:	80mmHg
Voltage:	230V-50/60Hz
Power:	200W





10711A0005/05/20/812





POSTHARVEST/02/20/11/11

  
**Biovopeak**

-  **Warning**  
Avoid contact with the interior of the oven when it is hot. Do not touch the interior.
-  **Dangerous**  
Do not touch the interior of the oven when it is hot.
-  **Note**  
The oven must be used in a well-ventilated area.
-  **Note**  
Do not touch the interior of the oven when it is hot.

**DRYING OVEN**

CEM-50-2L  






CENHBR-1L

mrc

10/10/2010 10:10:10



  
Biovopeak

-  **Dangerous**  
Never put inflammable and explosive organic solvent
-  **Note**  
Please do not put the volatile matter when working
-  **Note**  
Operation should avoid to be over-heated when working

FUTRN/ACMPS/06/20/004


INCUBATOR



INCUBATOR





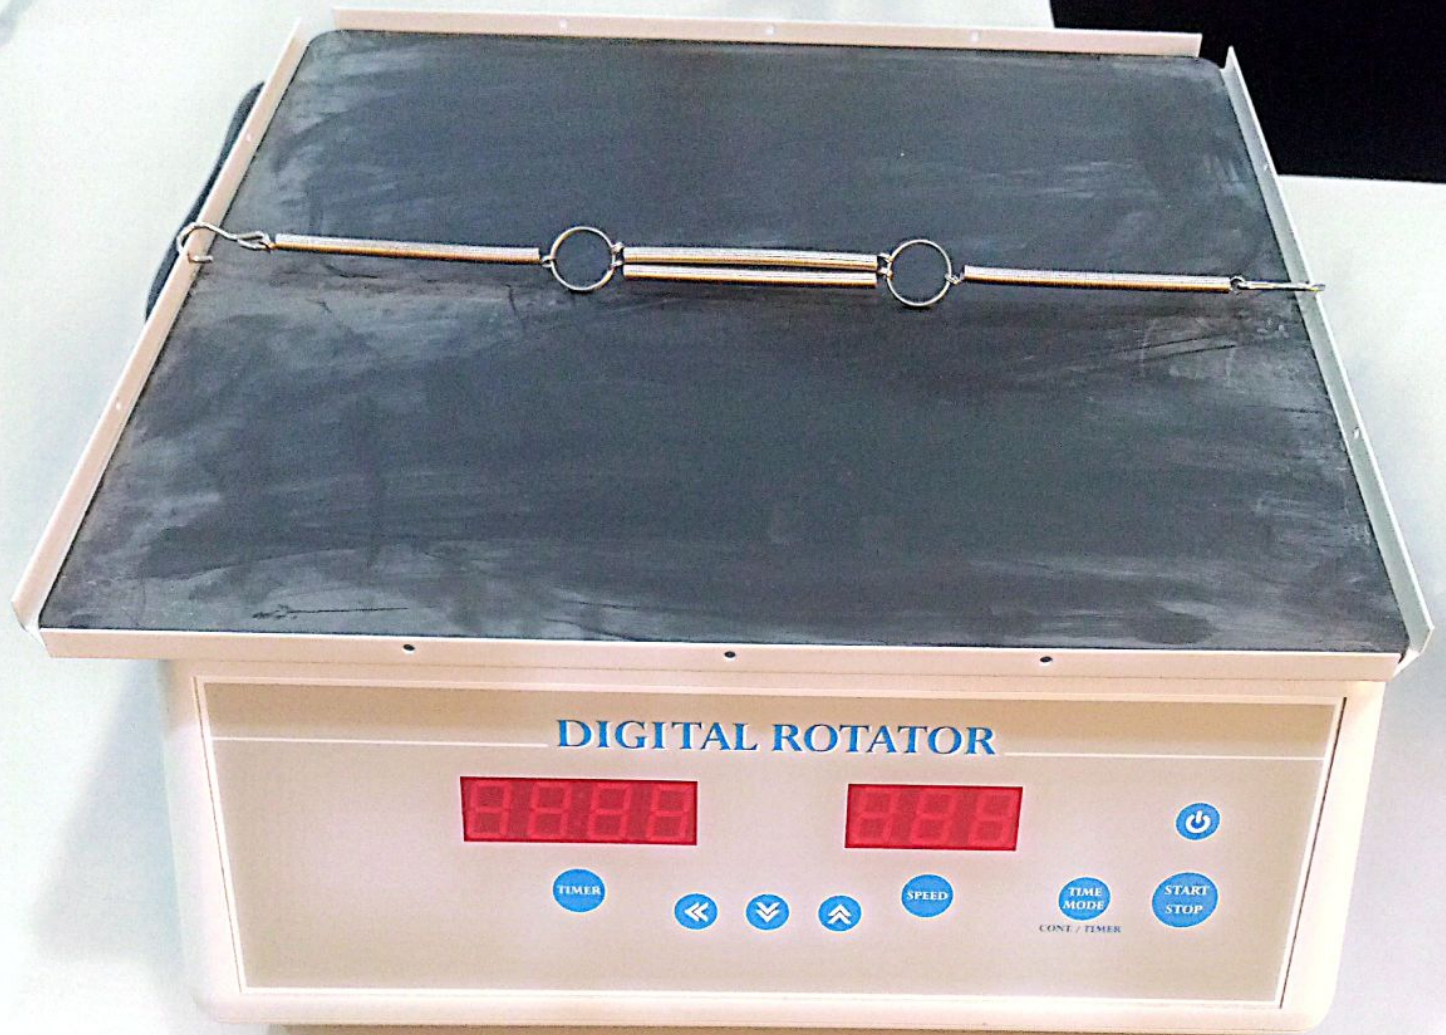

DIGITAL ROTATOR

8888

888

TIMER



SPEED

TIME MODE

CONT / TIMER

START STOP







FUTURA





VERTICAL STEAM STERILIZER

TEMPERATURE: 0000 TIME (min): 000

FUNCTION: [Blue button] [Blue button] [Blue button] [Blue button] [Blue button] [Blue button]

POWER ON [Green button]

  
Biovopeak












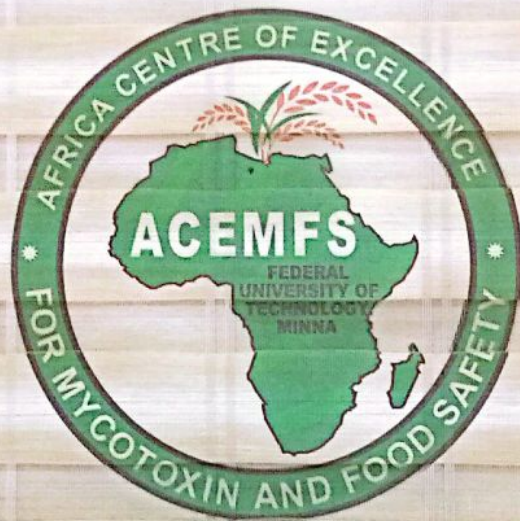











FOR ALL APPLIANCES OF 10000VA

**BLUE GATE**



INPUT VOLTAGE



OUTPUT VOLTAGE

NORMAL  
OVERVOLT  
LACKVOLT

**ZTY-10KVA**  
AC.AUTOMATIC VOLTAGE REGULATOR












CAPACITY  
35 KVA



**GENTO**  
House of Green Energy

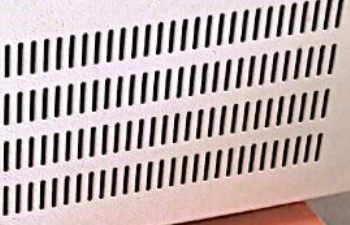

HYDRA ENERGY 12V 200AH







RACK 001

ENTO



